


-15kV TOF: -9245 v  
 -3.6kV MCP: -3364 v  
 -2.4kV MCP: -1774 v  
 Input Cur: 298 ma  
 RPA max: 237 v  
 Mirror max: 238 v

Wed Nov 29 10:39:55 2006

## TIDE Direct Events

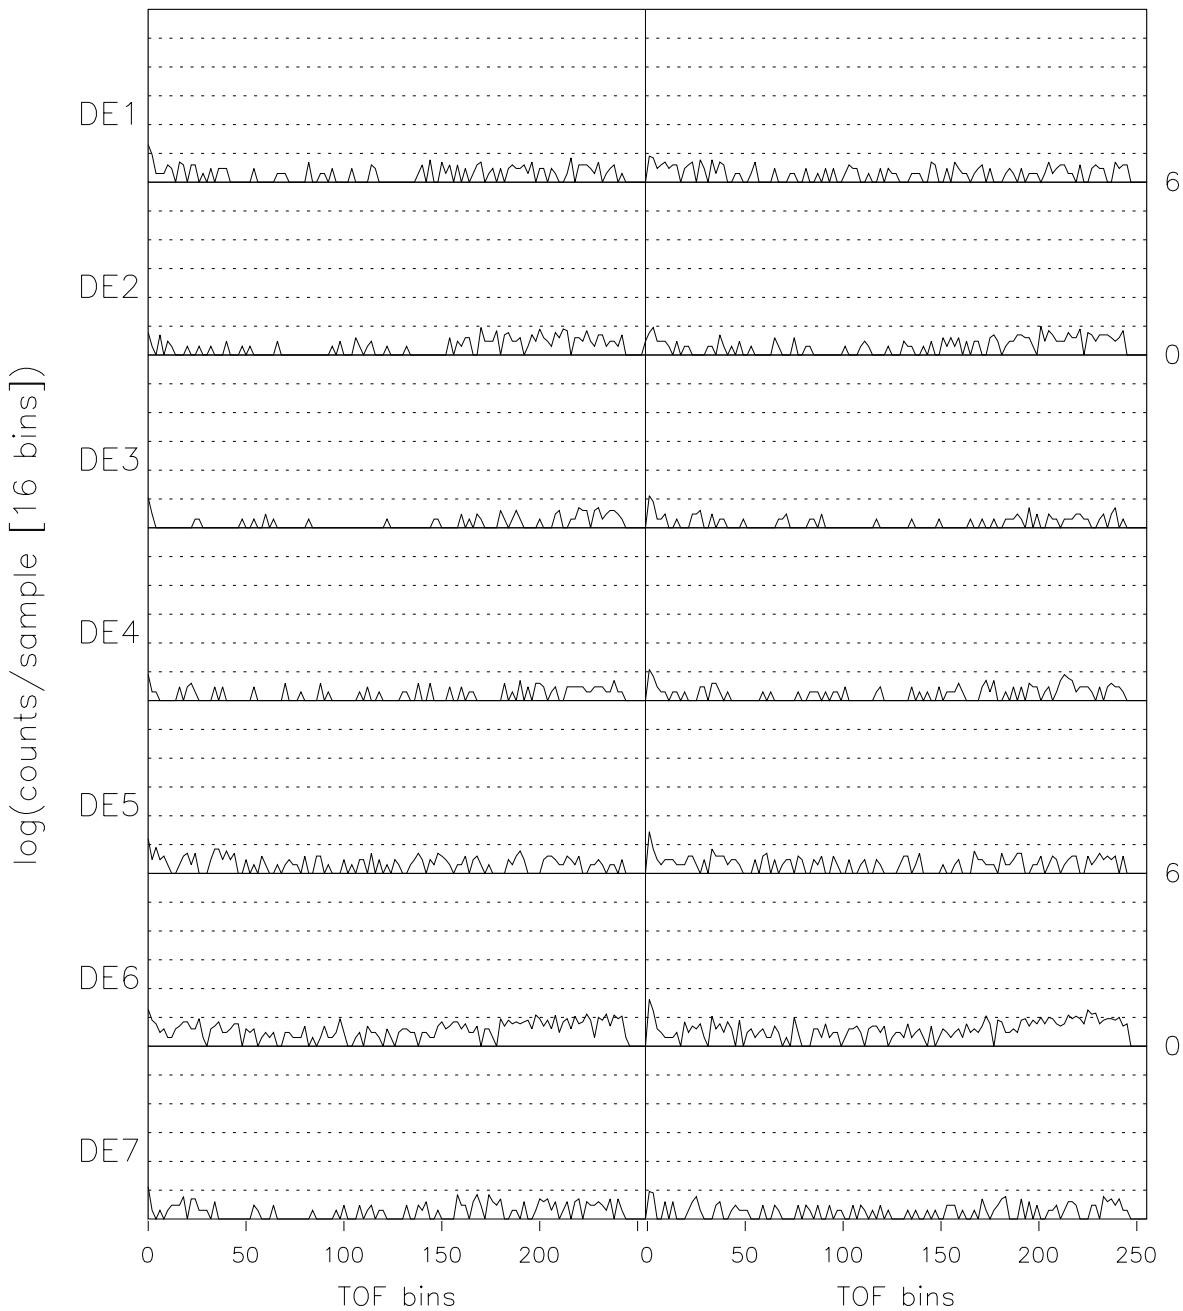

reported: 11-23-06 08:30:08 UT

reported: 11-23-06 08:33:20 UT

file: /export/data/tide/nrt/06112301.dat

-15kV TOF: -9245 v

-3.6kV MCP: -3379 v

-2.4kV MCP: -1774 v

Input Cur: 308 ma

RPA max: 237 v

Mirror max: 238 v